Application Note: Exhaust Fan Wiring Diagram

For ESRAD CO2 & Oxygen Safety Meters with 120VAC Relays

Notes:

This diagram shows the connections required to control a 120VAC exhaust fan from any of our wall-mounted ESRAD safety monitors and alarms.

The same diagram can be used to connect any of our meters, transmitters or wall monitors that include on on-board 120VAC, 3A, normally open (NO) relay.

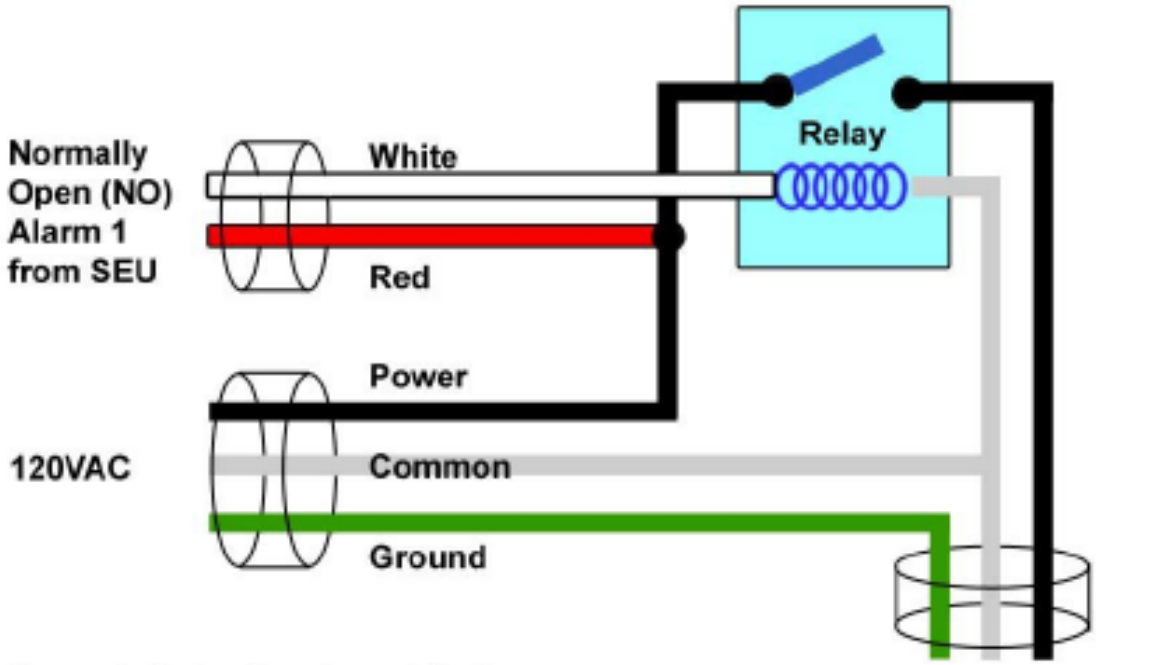

Example Relay Purchased Online:
Model 2W928 10A, 120VAC DPDT Relay
Model 10E075 Square Relay Socket

edaphic scientific
environmental research & monitoring equipment

Distributed & Supported By:
Edaphic Scientific Pty Ltd
www.edaphic.com.au
info@edaphic.com.au
P: 1300 430 928